

Appendix D. Calibration Certificates



SUB-CONTRACTING REPORT

CONTACT	: KELVIN CHEUNG	WORK ORDER	: HK2614792
CLIENT	: MOTT MACDONALD HONG KONG LIMITED		
ADDRESS	: 3/F INTERNATIONAL TRADE TOWER, 348 KWUN TONG ROAD, KWUN TONG, KOWLOON, HONG KONG	SUB-BATCH	: 1
		DATE RECEIVED	: 13-APR-2026
		DATE OF ISSUE	: 24-APR-2026
PROJECT	: CALIBRATION/PERFORMANCE CHECK OF DUST METER	NO. OF SAMPLES	: 1
		CLIENT ORDER	: ---

General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
 - Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
 - Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
 - Calibration was subcontracted to and analysed by Action-United Environmental Services & Consulting (AUES).
-

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

WORK ORDER : HK2614792
SUB-BATCH : 1
CLIENT : MOTT MACDONALD HONG KONG LIMITED
PROJECT : CALIBRATION/PERFORMANCE CHECK OF DUST METER



ALS Lab ID	Client's Sample ID	Sample Type	Sample Date	External Lab Report No.
HK2614792-001	S/N:597337	Equipments	13-Apr-2026	S/N:597337

----- END OF REPORT -----

Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust monitor
 Manufacturer: Sibata LD-3B
 Serial No. 597337
 Equipment Ref: Nil
 Job Order HK2614792

Standard Equipment:

Standard Equipment: Higher Volume Sampler
 Location & Location ID: AUES office (calibration room)
 Equipment Ref: HVS 018 (TISCH Model TE-5170X S/N:1260)
 Last Calibration Date: 27 March 2026


Equipment Verification Results:

Testing Date: 17 & 20 April 2026

Hour	Time	Mean Temp °C	Mean Pressure (hPa)	Concentration in µg/m ³ (Standard Equipment)	Total Count (Calibrated Equipment)	Count/Minute (Total Count/min)
2hr00min	09:50 ~ 11:50	25.2	1010.5	32.0	1583	13.1
2hr00min	11:58 ~ 13:58	25.2	1010.5	26.8	1529	12.7
2hr00min	14:00 ~ 16:00	25.2	1010.5	33.8	1902	15.9
2hr00min	09:36 ~ 11:36	26.7	1009.3	37.3	2023	16.9
2hr00min	11:41 ~ 13:41	26.7	1009.3	36.3	2236	18.6

Linear Regression of Y or X

Slope (K-factor): 2.0729 (µg/m³)/CPM
 Correlation Coefficient (R) 0.9856
 Date of Issue 24 April 2026

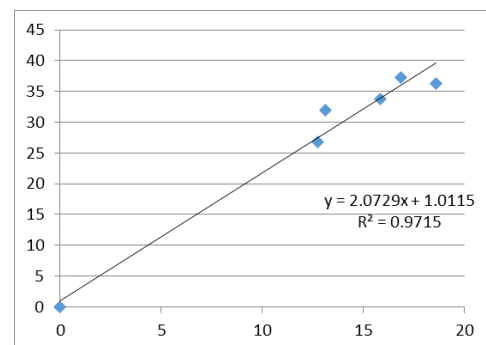

Remarks:

- Strong** Correlation (R>0.8)
- Factor 2.0729 (µg/m³)/CPM should be applied for TSP monitoring

*If R<0.5, repair or re-verification is required for the equipment

Operator : Jeff Ip Signature : [Signature] Date : 24 April 2026

QC Reviewer : Ben Tam Signature : [Signature] Date : 24 April 2026

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location : Gold King Industrial Building, Kwai Chung Date of Calibration: 27-Mar-26
 Location ID : Calibration Room - TISCH Higher Volume Sampler (Model TE-5170X) S/N:1260 Next Calibration Date: 27-Jun-26

CONDITIONS

Sea Level Pressure (hPa)	1011.7	Corrected Pressure (mm Hg)	758.775
Temperature (°C)	24.2	Temperature (K)	297

CALIBRATION ORIFICE

Make->	TISCH	Qstd Slope ->	2.13603
Model->	5025A	Qstd Intercept ->	-0.04992
Calibration Date->	8-Dec-25	Expiry Date->	8-Dec-26

CALIBRATION

Plate No.	H2O (L) (in)	H2O (R) (in)	H2O (in)	Qstd (m3/min)	I (chart)	IC corrected	LINEAR REGRESSION		
							Slope =	Intercept =	Corr. coeff. =
18	6.5	6.5	13.0	1.712	52	52.03	Slope =	30.7574	
13	5.2	5.2	10.4	1.534	46	46.02	Intercept =	-0.9552	
10	4.1	4.1	8.2	1.365	41	41.02	Corr. coeff. =	0.9992	
8	2.6	2.6	5.2	1.092	32	32.02			
5	1.6	1.6	3.2	0.861	26	26.01			

Calculations :

$$Q_{std} = 1/m[\text{Sqrt}(H2O(Pa/P_{std})(T_{std}/T_a)) - b]$$


$$IC = I[\text{Sqrt}(Pa/P_{std})(T_{std}/T_a)]$$

Qstd = standard flow rate
 IC = corrected chart responses
 I = actual chart response
 m = calibrator Qstd slope
 b = calibrator Qstd intercept
 Ta = actual temperature during calibration (deg K)
 Pstd = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I)[\text{Sqrt}(298/T_{av})(P_{av}/760)] - b)$$

m = sampler slope
 b = sampler intercept
 I = chart response
 Tav = daily average temperature
 Pav = daily average pressure

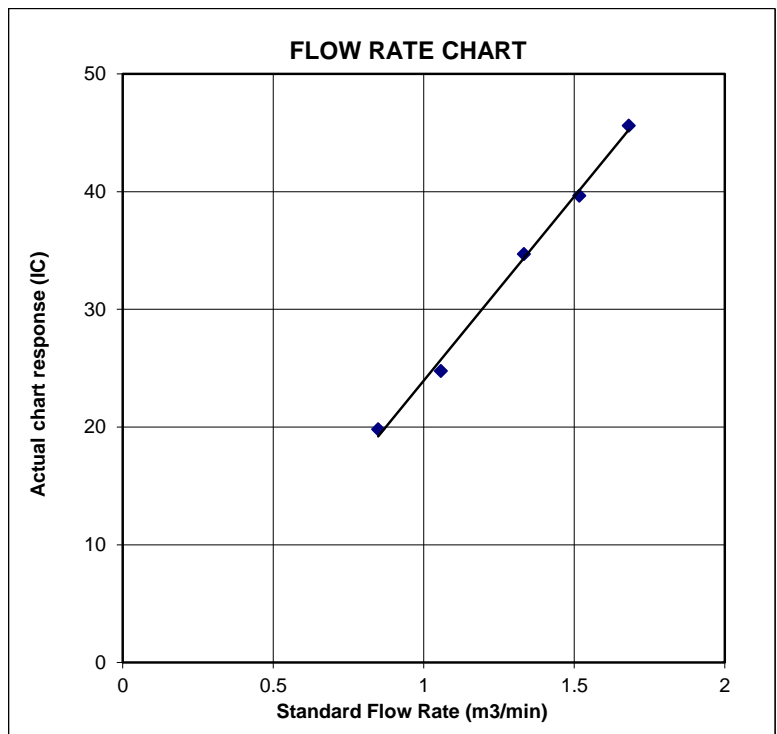



Certificate of Calibration

Calibration Certification Information			
Cal. Date: December 8, 2025	Rootsmeter S/N: 438320	Ta: 294	°K
Operator: Jim Tisch		Pa: 755.7	mm Hg
Calibration Model #: TE-5025A	Calibrator S/N: 1941		

Run	Vol. Init (m3)	Vol. Final (m3)	ΔVol. (m3)	ΔTime (min)	ΔP (mm Hg)	ΔH (in H2O)
1	1	2	1	1.4570	3.2	2.00
2	3	4	1	1.0380	6.4	4.00
3	5	6	1	0.9290	7.9	5.00
4	7	8	1	0.8850	8.8	5.50
5	9	10	1	0.7320	12.8	8.00

Data Tabulation						
Vstd (m3)	Qstd (x-axis)	$\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis)	Va	Qa (x-axis)	$\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis)	
1.0035	0.6888	1.4197	0.9958	0.6834	0.8821	
0.9993	0.9627	2.0078	0.9915	0.9552	1.2475	
0.9973	1.0735	2.2448	0.9895	1.0652	1.3948	
0.9961	1.1255	2.3543	0.9884	1.1168	1.4628	
0.9907	1.3535	2.8394	0.9831	1.3430	1.7642	
QSTD	m=	2.13603	QA	m=	1.33754	
	b=	-0.04992		b=	-0.03102	
	r=	1.00000		r=	1.00000	

Calculations			
Vstd=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$	Va=	$\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$
Qstd=	Vstd/ΔTime	Qa=	Va/ΔTime
For subsequent flow rate calculations:			
Qstd=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$	Qa=	$1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$

Standard Conditions	
Tstd:	298.15 °K
Pstd:	760 mm Hg
Key	
ΔH:	calibrator manometer reading (in H2O)
ΔP:	rootsmeter manometer reading (mm Hg)
Ta:	actual absolute temperature (°K)
Pa:	actual barometric pressure (mm Hg)
b:	intercept
m:	slope

RECALIBRATION
US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30